

Repair ticket

Flexible Endoscope

Olympus®, Pentax®, Fujinon®, diverse



emos
technology

Servicenummer: _____

Gültig ab:
23.01.2024

Freigabe
Nathalie Faschian

Revision
B

FB-1907 – Page 2

DCN 148

Dear Customer,

to ensure your request the fastest possible, please describe the reason for the repair as precisely as possible.

Address (stamp if necessary)

Name: _____

Street: _____

Postal code, City: _____

Device type

Manufacturer: _____

Type/Art.-No.: _____

Serial number: _____

Repair It is a loaner device

Flexible Endoscope (please tick applicable defect)

Valves / function buttons

- leaking
- disturbed

A/W insufflation

- disturbed

Instrument channel

- leaking
- constricted

Insertion tube

- kinked
- leaking
- surface damaged

Distal end

- lenses / optics
- nozzles

Ocular

- leaking
- foggy
- image disturbed

Angulation wheels

- tolerance
- leaking

Control body

- leaking

Light guide connector

- leaking

Angulation

- insufficient
- sleeve leaking

Electronics


- CCD-problems
- image disturbed
-

Supply tube

- kinked
- leaking

Optical fiber

- broken
- light output

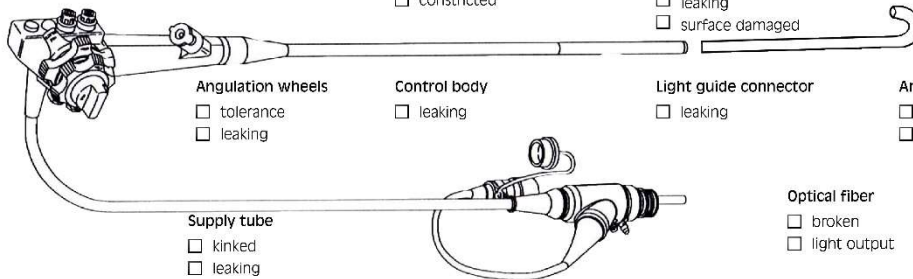

Remarks / Error description

Safety information for the protection of employees

Decontamination certificate (please mark with a cross)



In the Medical Device Law Implementation Act (MPDG) and in the reprocessing of healthcare products (DIN EN ISO 17664) contain various legal requirements for the reprocessing of used medical devices. Since these medical devices can be a source of infections in humans, proper and professional reprocessing of these medical devices is an indispensable must.

Yes, the product is manually disinfected. Name, employees: _____

Yes, the products is mechanical disinfected. Batch-No.: _____

No, the product is not disinfected*. Reason: _____

Please mark on the outer package that device is contaminated!

I hereby confirm the accuracy of all information:

Name: _____ Date: _____ Signature: _____

Thank you very much for your assistance!
Your EMOS- Team